



Client Redacted Research FL **Analyzed** 08/10/2026

This Certificate of Analysis certifies that the sample listed herein was tested by SteriGenix using validated analytical methods and was found to meet the stated specifications at the time of analysis.

SAMPLE INFORMATION

Product	Tesamorelin	Form	Lyophilized
Batch	SGX-RRFL-2026-0727-M46	Labeled Qty	10MG
Mol. Formula	C221H366N72O67S	CAS Number	218949-48-5
Cap Color	White	Crimp Color	Silver
Appearance	White Powder		

TEST RESULTS

	REFERENCE STANDARD	RESULT	
Identity Confirmation (LC-MS)	Tesamorelin	Tesamorelin	✓
Batch Avg Purity (HPLC)	(>98%)	99.48	✓
Net Peptide Content	10MG ± 10%	10.36	✓

HEAVY METAL SCREENING


No data.

BATCH CONFORMITY RESULTS

No data.

HPLC CHROMATOGRAM

HPLC CHROMATOGRAM · TESAMORELIN 10MG	DETECTOR: UV 214 NM · 08/10/2026

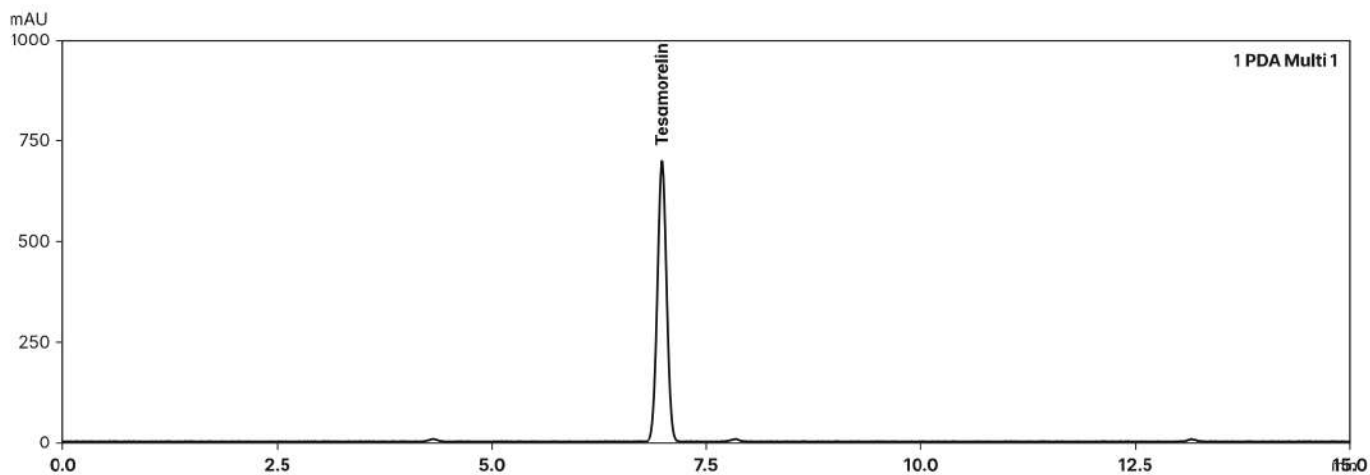

SAMPLE PHOTOS



AS RECEIVED

RECONSTITUTED (BACT. WATER) — CLARITY
CHECK

Dr. R. Caldwell

ANALYST
ID: AN-3271

Dr. P. Andersen

QC REVIEWER
ID: QR-5418

Dr. H. Whitman

QA DIRECTOR
ID: QA-1090



sterigenixanalytical.com/verify

Report#: RPT-2026-100313

Access Code: SGX-RRFL-2026-0727-M46



Client Redacted Research FL **Analyzed** 08/10/2026

This Certificate of Analysis certifies that the sample listed herein was tested by SteriGenix using validated analytical methods and was found to meet the stated specifications at the time of analysis.

SAMPLE INFORMATION

Product	Tesamorelin	Form	Lyophilized
Batch	SGX-RRFL-2026-0727-R06	Labeled Qty	20MG
Mol. Formula	C221H366N72O67S	CAS Number	218949-48-5
Cap Color	Blue	Crimp Color	Silver
Appearance	White Powder		

TEST RESULTS

	REFERENCE STANDARD	RESULT	
Identity Confirmation (LC-MS)	Tesamorelin	Tesamorelin	✓
Batch Avg Purity (HPLC)	(>98%)	99.47	✓
Net Peptide Content	20MG ± 10%	20.74	✓

HEAVY METAL SCREENING


No data.

BATCH CONFORMITY RESULTS



No data.

HPLC CHROMATOGRAM

HPLC CHROMATOGRAM · TESAMORELIN 20MG	DETECTOR: UV 214 NM · 08/10/2026

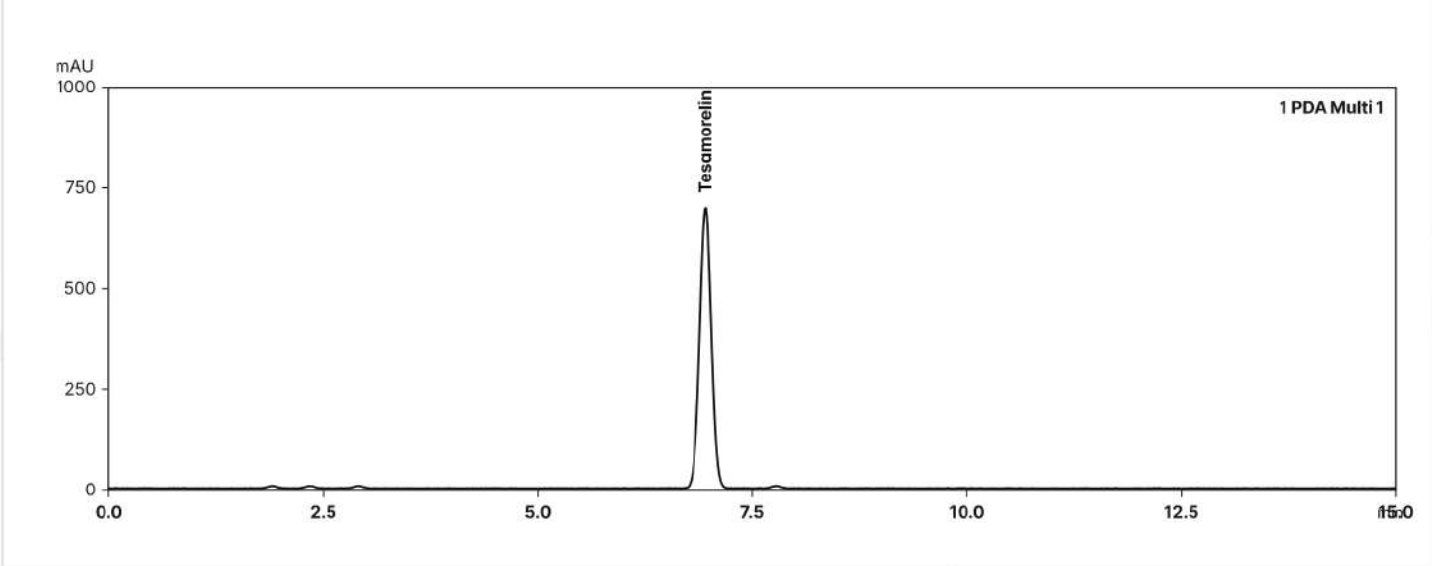

SAMPLE PHOTOS

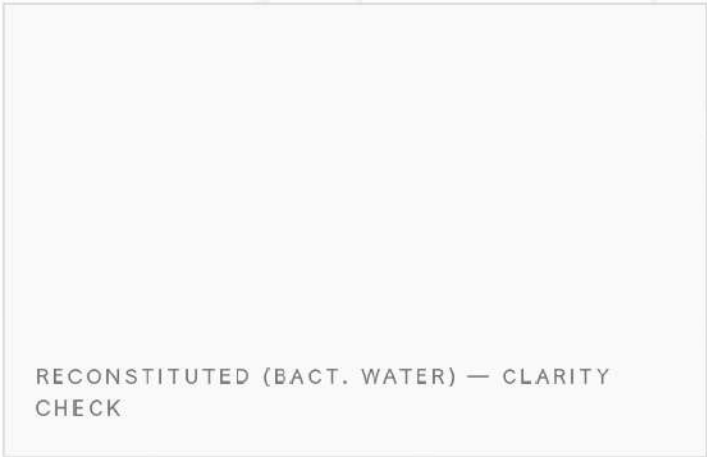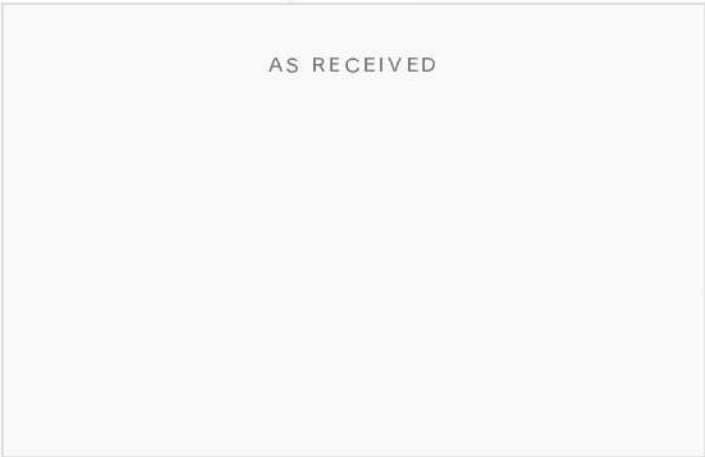

Dr. R. Caldwell
ANALYST
ID: AN-3271

Dr. P. Andersen
QC REVIEWER
ID: QR-5418

Dr. H. Whitman
QA DIRECTOR
ID: QA-1090



sterigenixanalytical.com/verify

Report#: RPT-2026-100330
Access Code: SGX-RRFL-2026-0727-R06