



Client Redacted Research FL **Analyzed** 08/10/2026

This Certificate of Analysis certifies that the sample listed herein was tested by SteriGenix using validated analytical methods and was found to meet the stated specifications at the time of analysis.

SAMPLE INFORMATION

Product	Tirzepatide	Form	Lyophilized
Batch	SGX-RRFL-2026-0727-X45	Labeled Qty	20MG
Mol. Formula	C225H348N48O68	CAS Number	2023788-19-2
Cap Color	Blue	Crimp Color	Silver
Appearance	White Powder		

TEST RESULTS

	REFERENCE STANDARD	RESULT	
Identity Confirmation (LC-MS)	Tirzepatide	Tirzepatide	✓
Batch Avg Purity (HPLC)	(>98%)	99.76	✓
Net Peptide Content	20MG ± 10%	20.89	✓

HEAVY METAL SCREENING


No data.

BATCH CONFORMITY RESULTS



No data.

HPLC CHROMATOGRAM

HPLC CHROMATOGRAM · TIRZEPATIDE 20MG	DETECTOR: UV 214 NM · 08/10/2026

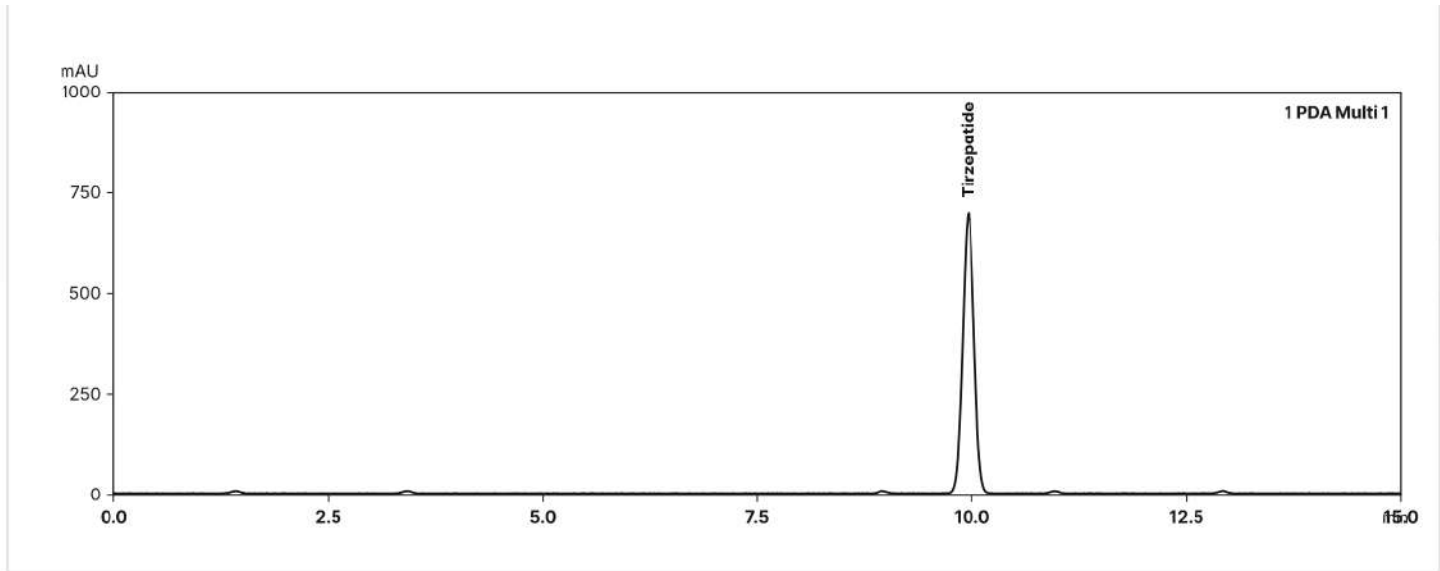

SAMPLE PHOTOS

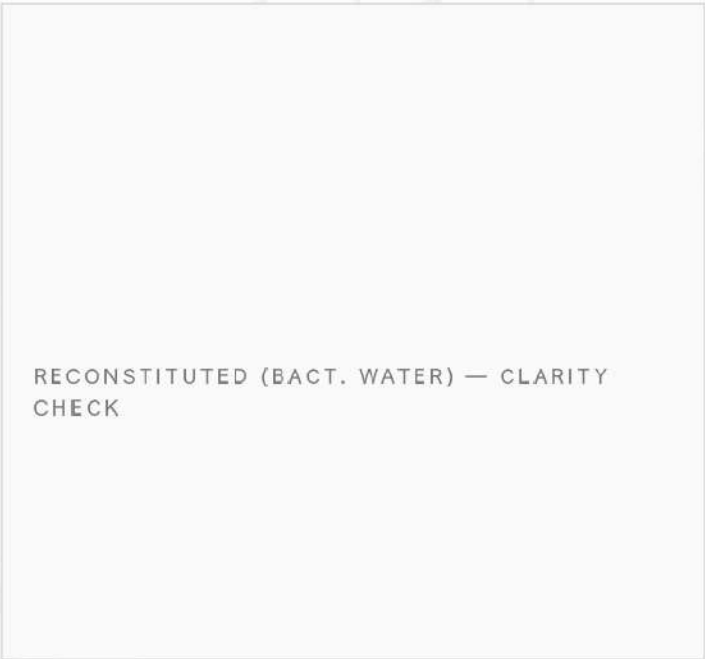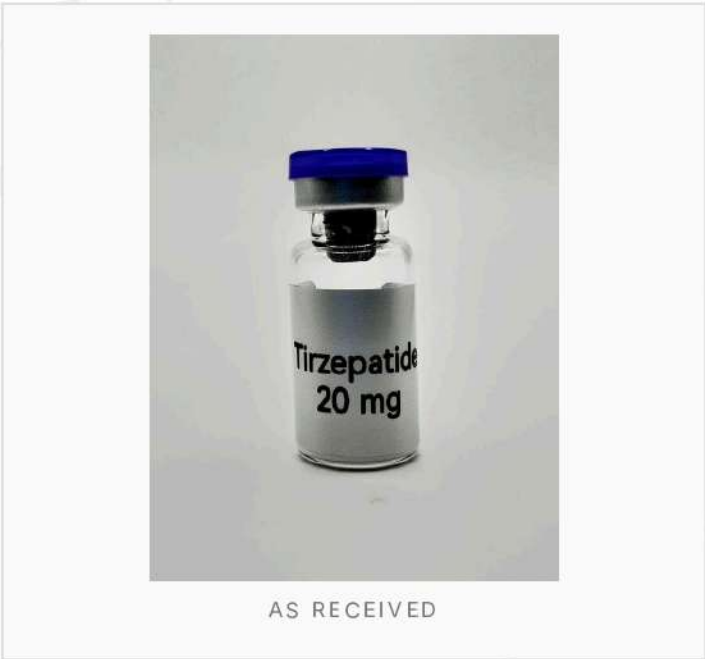

Dr. R. Caldwell
ANALYST
ID: AN-3271

Dr. P. Andersen
QC REVIEWER
ID: QR-5418

Dr. H. Whitman
QA DIRECTOR
ID: QA-1090



sterigenixanalytical.com/verify

Report#: RPT-2026-100347
Access Code: SGX-RRFL-2026-0727-X45



Client Redacted Research FL **Analyzed** 08/10/2026

This Certificate of Analysis certifies that the sample listed herein was tested by SteriGenix using validated analytical methods and was found to meet the stated specifications at the time of analysis.

SAMPLE INFORMATION

Product	Tirzepatide	Form	Lyophilized
Batch	SGX-RRFL-2026-0727-S63	Labeled Qty	30MG
Mol. Formula	C225H348N48O68	CAS Number	2023788-19-2
Cap Color	Pink	Crimp Color	Silver
Appearance	White Powder		

TEST RESULTS

	REFERENCE STANDARD	RESULT	
Identity Confirmation (LC-MS)	Tirzepatide	Tirzepatide	✓
Batch Avg Purity (HPLC)	(>98%)	99.51	✓
Net Peptide Content	30MG ± 10%	30.44	✓

HEAVY METAL SCREENING


No data.

BATCH CONFORMITY RESULTS



No data.

HPLC CHROMATOGRAM

HPLC CHROMATOGRAM · TIRZEPATIDE 30MG	DETECTOR: UV 214 NM · 08/10/2026

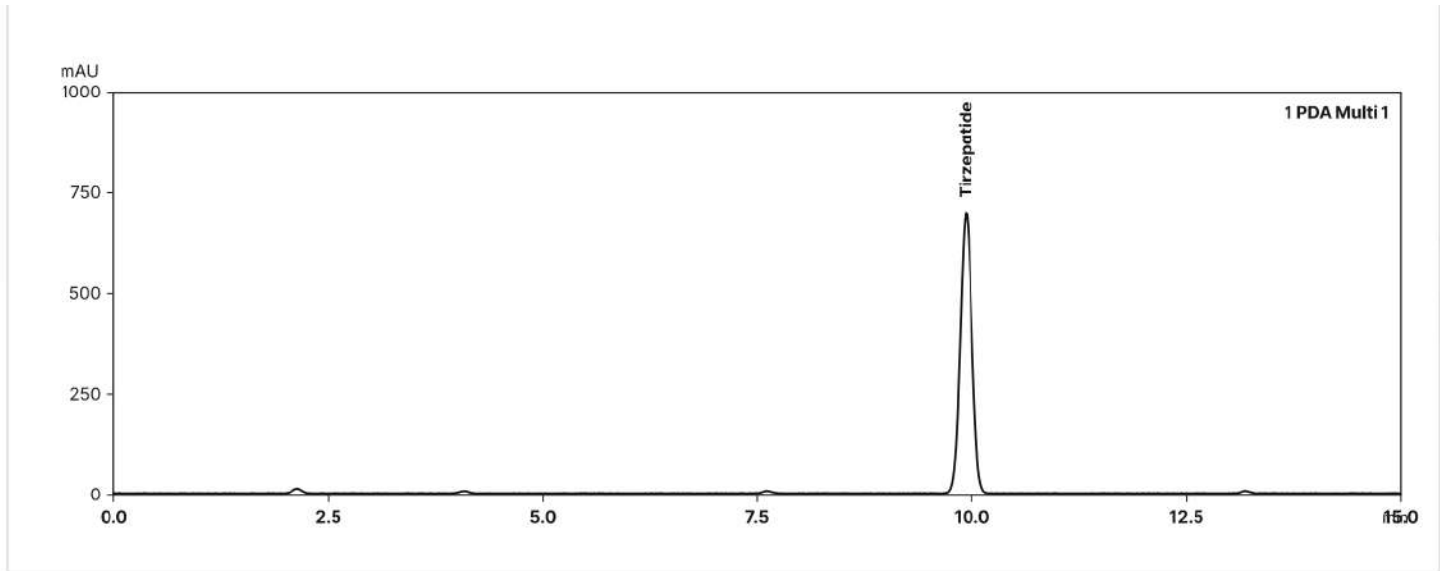

SAMPLE PHOTOS

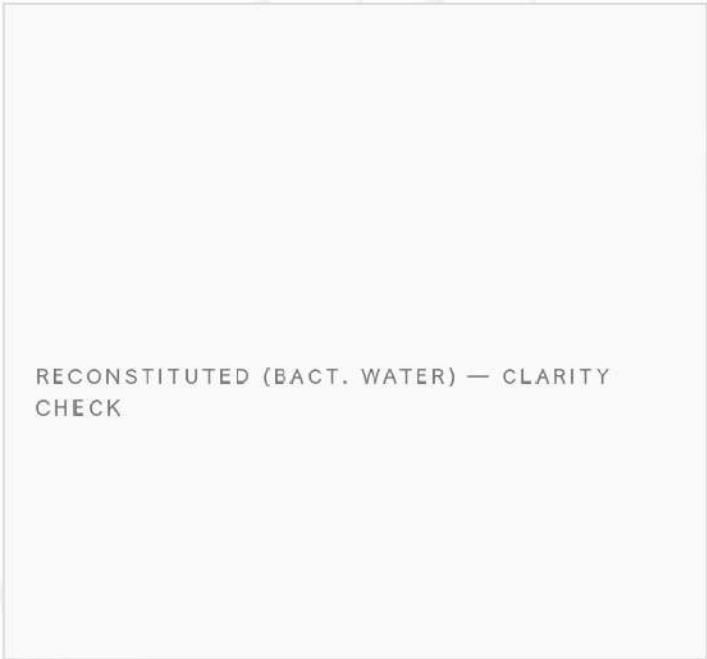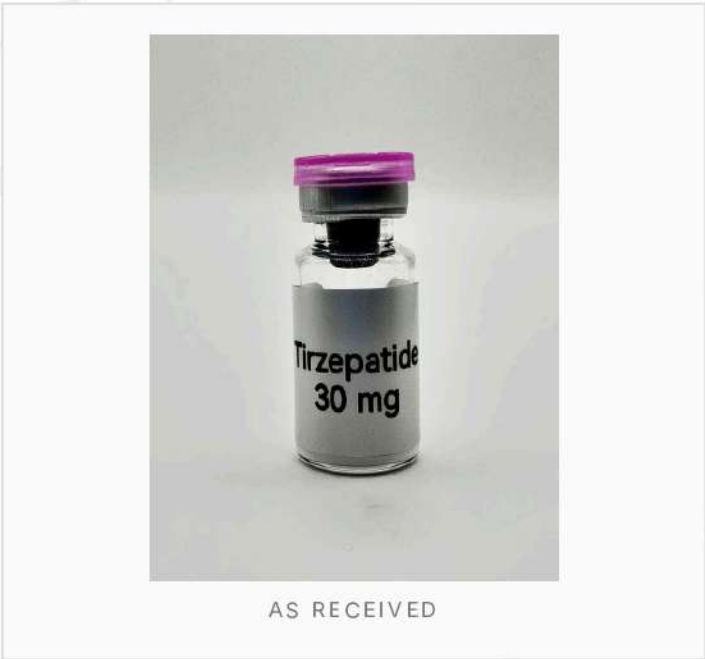

Dr. R. Caldwell
ANALYST
ID: AN-3271

Dr. P. Andersen
QC REVIEWER
ID: QR-5418

Dr. H. Whitman
QA DIRECTOR
ID: QA-1090



sterigenixanalytical.com/verify

Report#: RPT-2026-100364
Access Code: SGX-RRFL-2026-0727-S63